

SUPERVISOR TEST




CARMEL TOWN
POLICE DEPT
DATAMASTER dmt: 100196

Date: 07/14/2020

OPERATOR NAME:
ROBERT BAGNAROL
Permit #: 43570
Operator Agency/Dept: CARMEL TOWN PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:52
INTERNAL STANDARD	VERIFIED	12:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:52
BLANK TEST	0.00	12:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:53
BLANK TEST	0.00	12:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	12:54
BLANK TEST	0.00	12:55

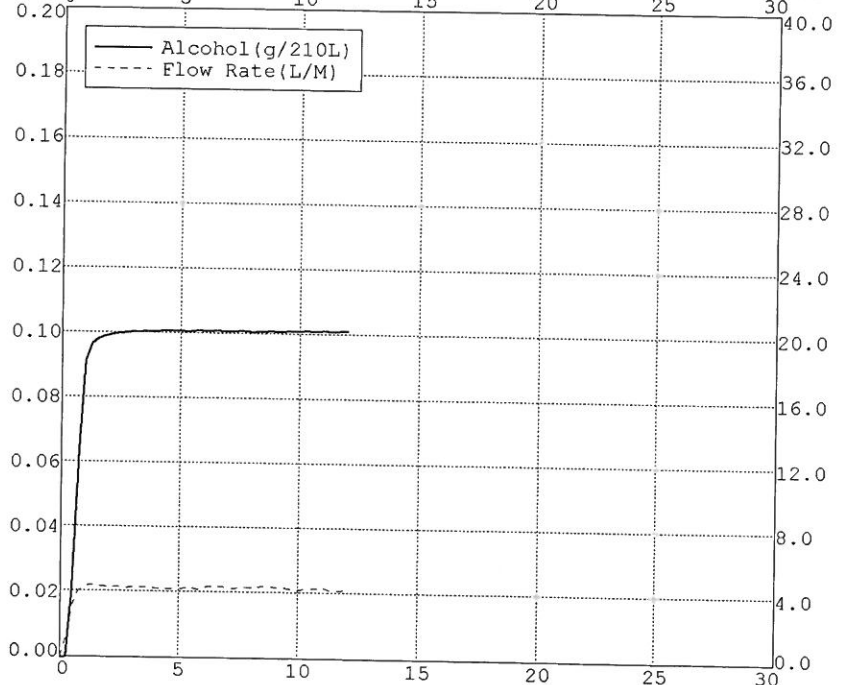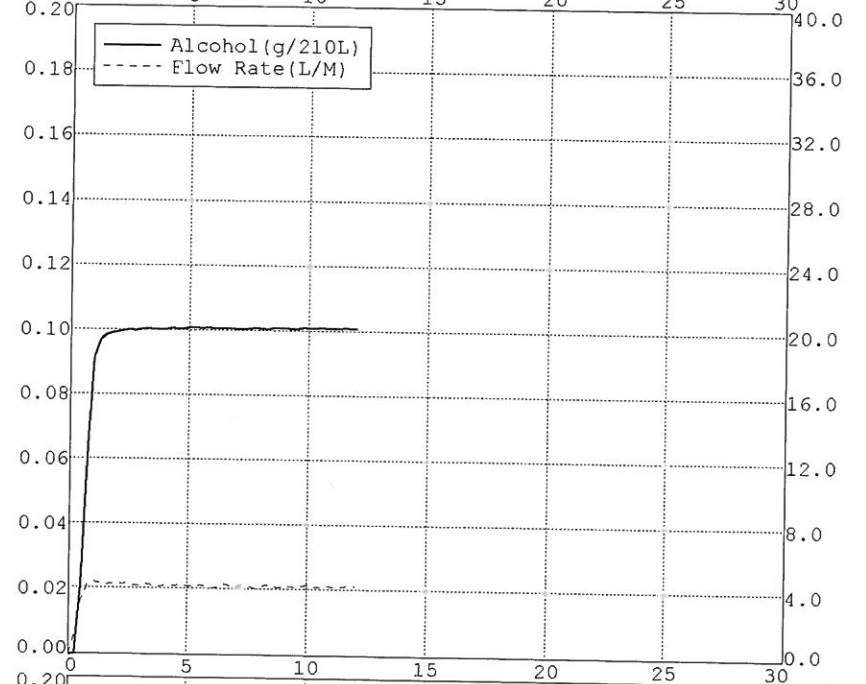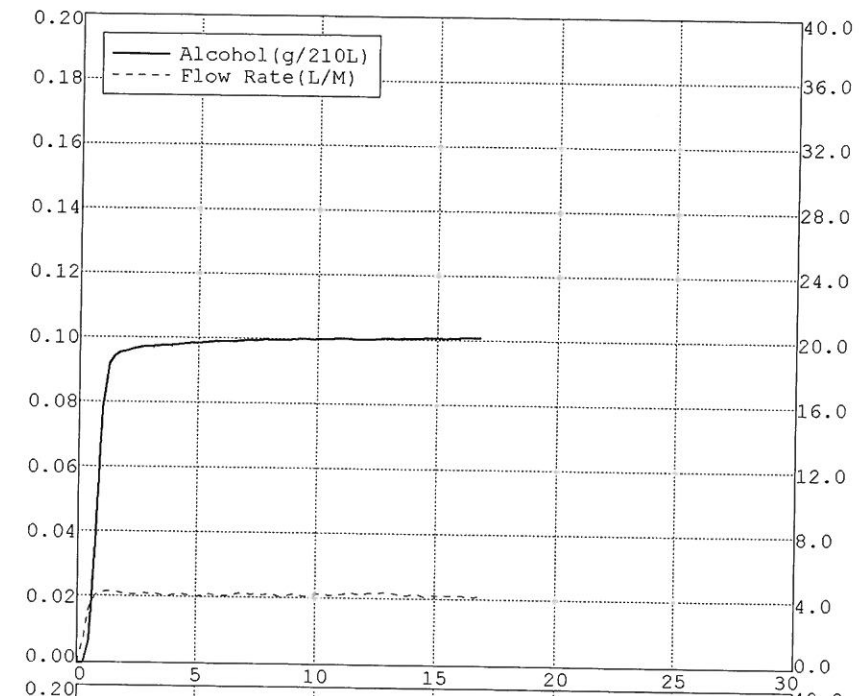

SUPERVISOR TEST

CARMEL TOWN
POLICE DEPT
DATAMASTER dmt: 100196

Date: 07/19/2020

OPERATOR NAME:
STEPHEN M MCCABE
Permit #: 41419
Operator Agency/Dept: CARMEL TOWN PD
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:34
INTERNAL STANDARD	VERIFIED	15:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:34
BLANK TEST	0.00	15:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	15:35
BLANK TEST	0.00	15:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:37
BLANK TEST	0.00	15:37

