

SOLUTION CHANGE




CARMEL TOWN
POLICE DEPT
DATAMASTER dmt: 100196

Date: 06/01/2023

OPERATOR NAME:
STEPHEN M MCCABE
Permit #: 41419
Operator Agency/Dept: CARMEL TOWN PD
Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:53
INTERNAL STANDARD	VERIFIED	23:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	23:54
BLANK TEST	0.00	23:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	23:55
BLANK TEST	0.00	23:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	23:56
BLANK TEST	0.00	23:57

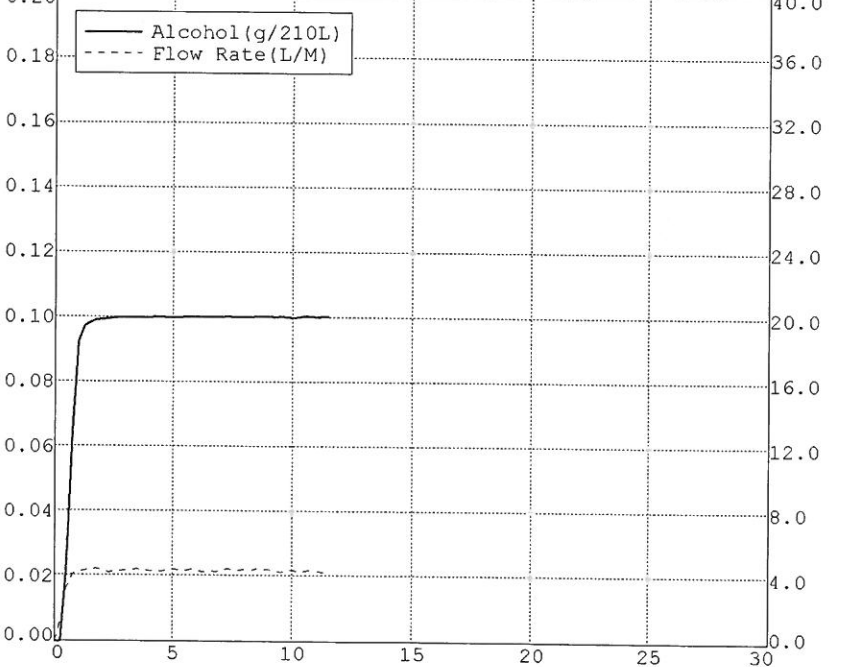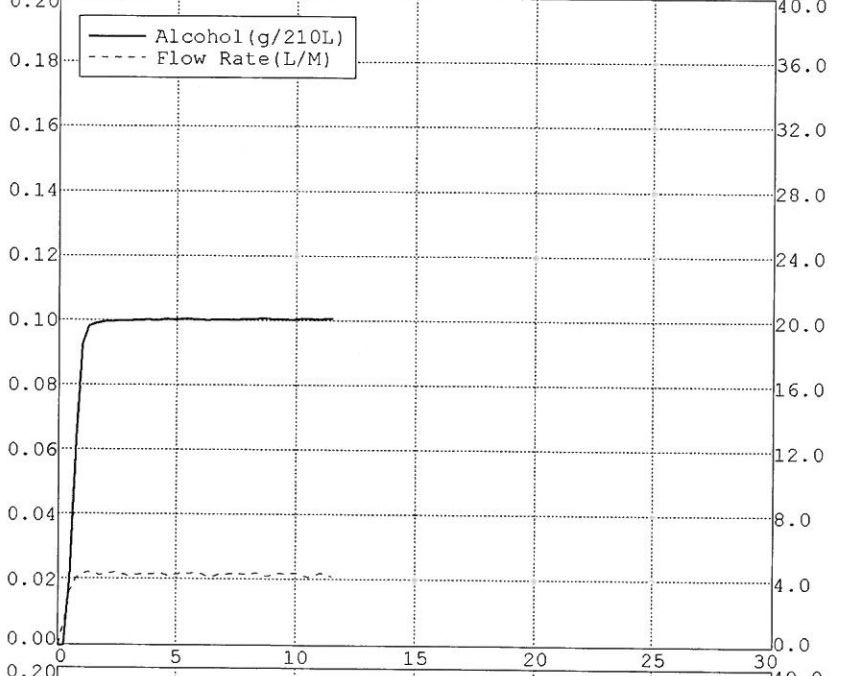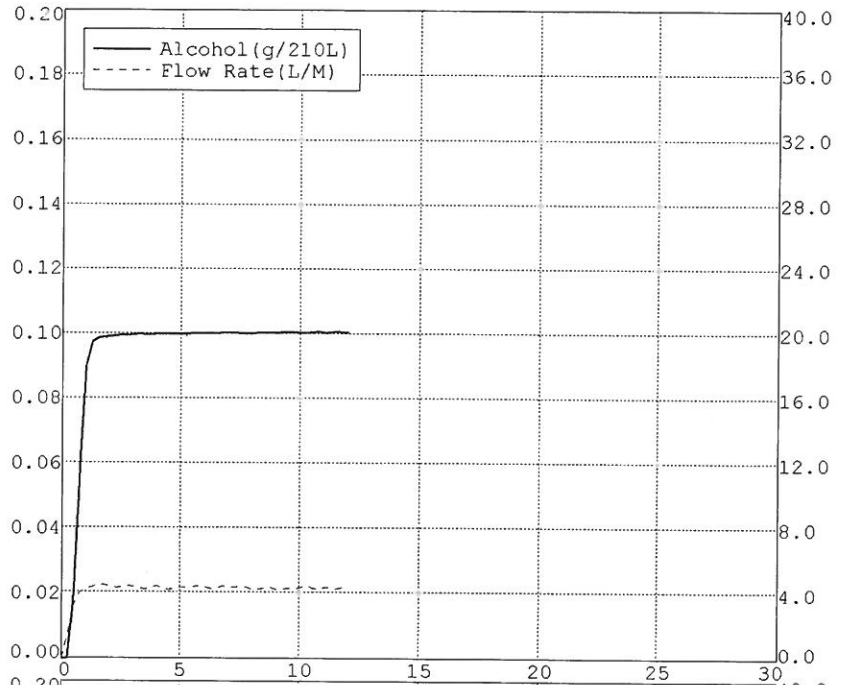

SOLUTION CHANGE

CARMEL TOWN
POLICE DEPT
DATAMASTER dmt: 100196

Date: 06/01/2023

OPERATOR NAME:
STEPHEN M MCCABE
Permit #: 41419
Operator Agency/Dept: CARMEL TOWN PD
Reference Standard #: 23090

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:50
INTERNAL STANDARD	VERIFIED	23:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	INTERFERENCE	23:50

Interference Detected

